


# Medtronic

Sonicision™ 7 curved jaw cordless ultrasonic dissector

# Cordless freedom to do more,<sup>1,†,‡,ΩΩ</sup> your way.

The next advancement<sup>†</sup> in cordless ultrasonic dissection is here – now designed to coagulate and dissect vasculature up to and including 7 mm in diameter.<sup>1,‡</sup>

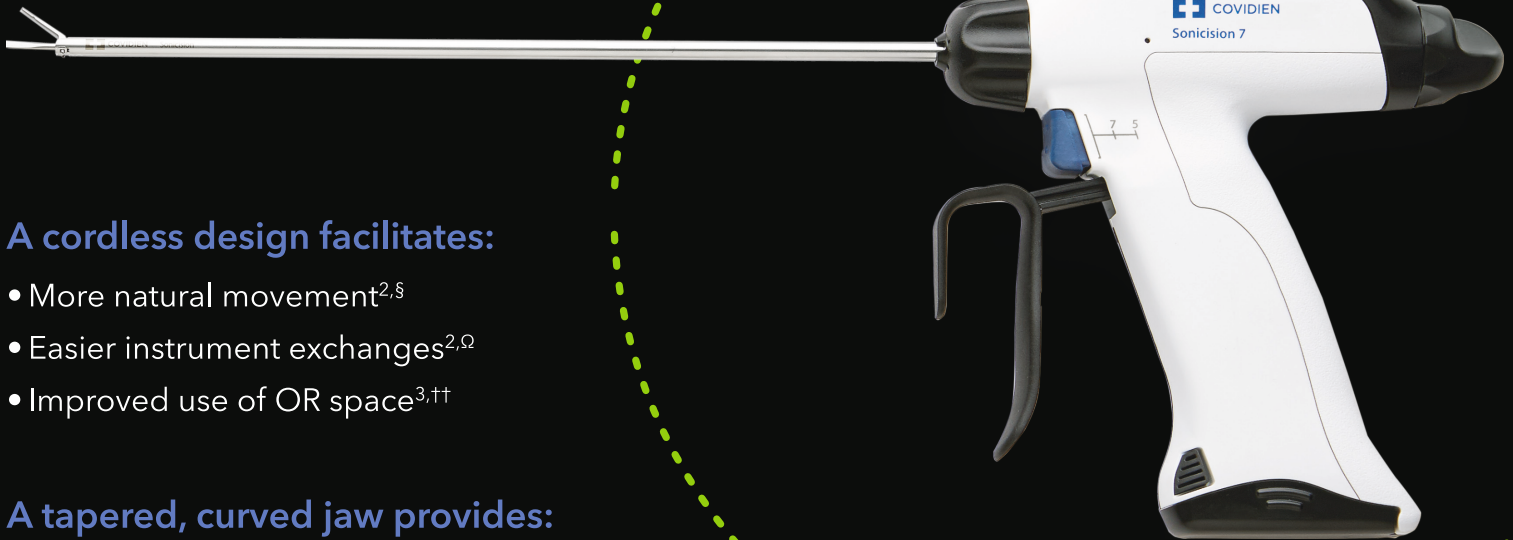

## A cordless design facilitates:

- More natural movement<sup>2,§</sup>
- Easier instrument exchanges<sup>2,Ω</sup>
- Improved use of OR space<sup>3,††</sup>

## A tapered, curved jaw provides:

- Access in tight spaces<sup>2,††</sup>
- Visualization of target structures<sup>2,††</sup>
- Precise energy dissection<sup>1,‡</sup>

## A single intuitive<sup>1,‡</sup> dual mode energy activation button enables:

- Procedural versatility<sup>1,§§</sup>
- The surgeon's eyes to stay on the surgical field<sup>1,ΩΩ</sup>
- Improved surgical efficiency<sup>1,‡</sup>

# The cordless freedom you expect with the advancements<sup>†</sup> you desire.

The Sonicision™ 7 curved jaw device remains the first and only cordless ultrasonic dissector. Now with the ability to coagulate and dissect vessels up to and including 7 mm in diameter.<sup>1,†</sup>



## Cordless power in the palm of your hand

A reusable generator enables:

- Use for **150 procedures** before replacement<sup>4</sup>
- **Streamlined<sup>†</sup> cleaning and sterilization** because it's autowashable and autoclavable

A reusable nonsterile battery pack provides:

- **88 percent greater capacity<sup>5,†</sup>** to instill confidence of consistent power throughout long procedures
- **200 procedural uses<sup>6,7</sup>** – twice the number of earlier devices<sup>†</sup>
- No-hassle power management via **a simple, intuitive charger<sup>3,†††</sup>**



## Ordering information

SCD7A13	Sonicision™ 7 curved jaw cordless ultrasonic dissector – 13 cm	6/case
SCD7A26	Sonicision™ 7 curved jaw cordless ultrasonic dissector – 26 cm	6/case
SCD7A39	Sonicision™ 7 curved jaw cordless ultrasonic dissector – 39 cm	6/case
SCD7A48	Sonicision™ 7 curved jaw cordless ultrasonic dissector – 48 cm	6/case
SCBA	Sonicision™ reusable battery pack	1/each
SCG7AB	Sonicision™ 7 reusable generator	1/each
SCBIGA	Sonicision™ reusable battery insertion guide	2/pack
CBCA	Sonicision™ battery charger	1/each
SCSTA	Sonicision™ reusable sterilization tray	1/each

Bring greater efficiency<sup>1,†</sup> and freedom of movement<sup>2,†††</sup> to your OR.

Call your Medtronic sales rep today or scan the below QR code



Call: 080 48971329  
Email: rs.indiainsidesales@medtronic.com

1261, Solitaire Corporate Park,  
Bldg. No. 12, 6th Floor,  
Andheri - Ghatkopar Link Road,  
Andheri (East), Mumbai - 400093

[medtronic.co.in](http://medtronic.co.in)

**Medtronic**

<sup>†</sup>Compared to earlier generations of the Sonicision™ curved jaw device. †25 out of 27 surgeons surveyed after use agreed. §30 out of 33 surgeons surveyed after use agreed. Ω32 out of 33 surgeons surveyed after use agreed. ††29 out of 29 nurses surveyed after use agreed. †††33 out of 33 surgeons surveyed after use agreed. §§27 out of 27 surgeons surveyed after use agreed. ΩΩ26 out of 27 surgeons surveyed after use agreed. †††28 out of 28 nurses surveyed after use agreed. ††††29 out of 33 surgeons surveyed after use agreed. 1. Based on internal test report #RE00329878 rev A, Marketing evaluation of surgeon experience using the Sonicision™ 7 curved jaw cordless ultrasonic dissector. Apr. 14-15 and 20-22, 2021. 2. Based on internal test report #R0042752 rev A, Marketing evaluation of surgeon experience using the Sonicision™ curved jaw cordless ultrasonic dissector. Feb. 13-17, Feb. 28, March 3, May 16, 2017. 3. Based on internal test report #R0049393 rev A, Operating room staff marketing evaluation of the Sonicision™ curved jaw cordless ultrasonic dissector. Dec. 1, 6-7, 2016. 4. Based on internal test report #RE00108733, rev A, Reusable life test verification report (SCGAA-TA9). August 24, 2017. 5. Based on internal test memo #RE00153542, rev B, Battery capacity comparison between SCB and SCBA. May 17, 2018. 6. Based on internal test report #R0042707, rev A, Reusable life test verification report for the SCBA reusable battery pack. April 26, 2017. 7. Based on internal test report #RE00113195, rev A, Reusable life test verification report for the SCBA reusable battery pack – Oxivir. September 13, 2017.